



# Pulse Damper Comparison

## Performance and Reliability

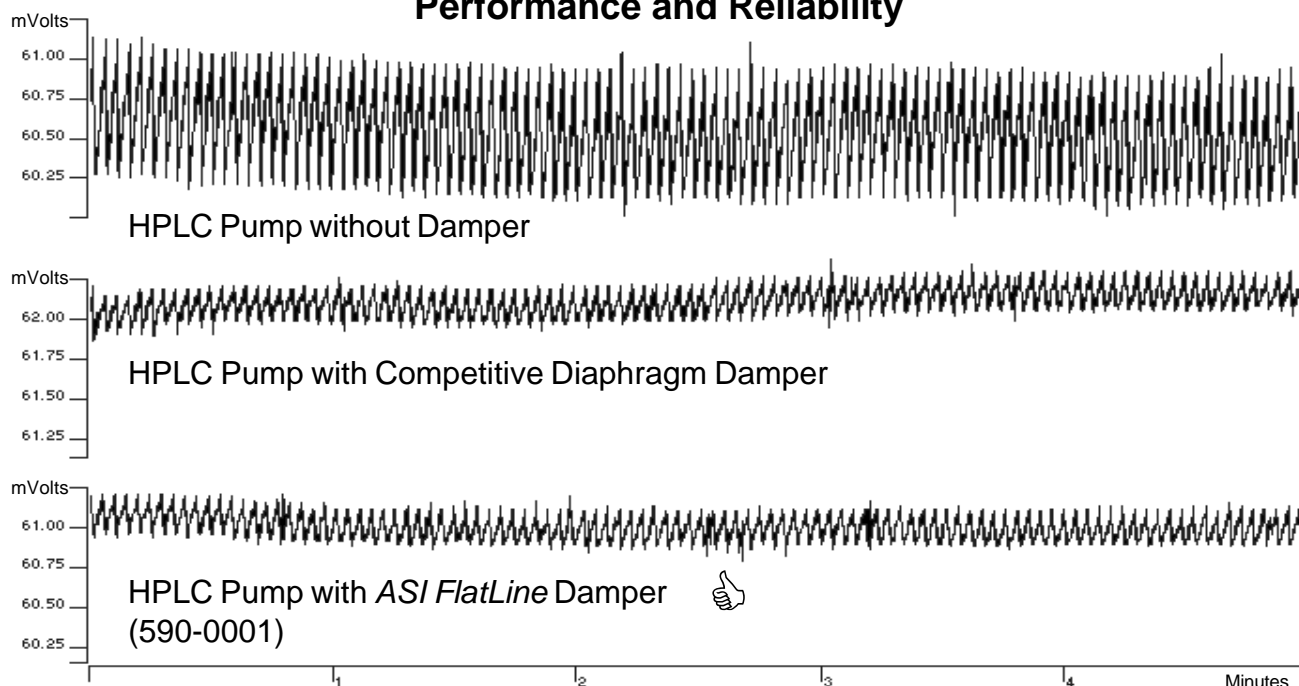

<b>HPLC System Configuration:</b> HPLC Pump Amplified Ext. Pressure Transducer Varian Star Data Acquisition	<b>HPLC Conditions:</b> MP: A = H <sub>2</sub> O Flow Rate: 1.0 mL/min. Isocratic Pressure: 2,300 PSI with restrictor
----------------------------------------------------------------------------------------------------------------------	--------------------------------------------------------------------------------------------------------------------------------

## Solid Core Design Improves Flush Out and Dispersion

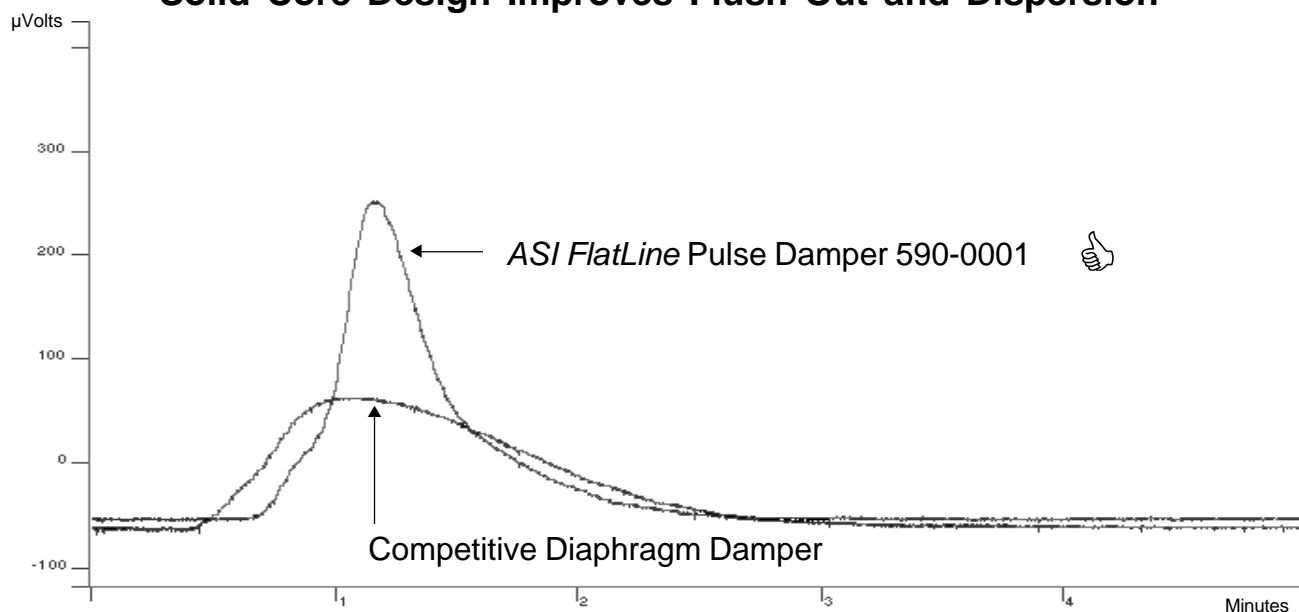

<b>HPLC System Configuration:</b> HPLC Pump ABI Model 785 UV/VIS @254 nm column Varian Star Data Acquisition	<b>HPLC Conditions:</b> MP: A = H <sub>2</sub> O Flow Rate: 1.0 mL/min. Isocratic Pressure: 2,300 PSI with restrictor Injection: 10 μL Acetone
-----------------------------------------------------------------------------------------------------------------------	------------------------------------------------------------------------------------------------------------------------------------------------------------